


Configuration of EXCAVA

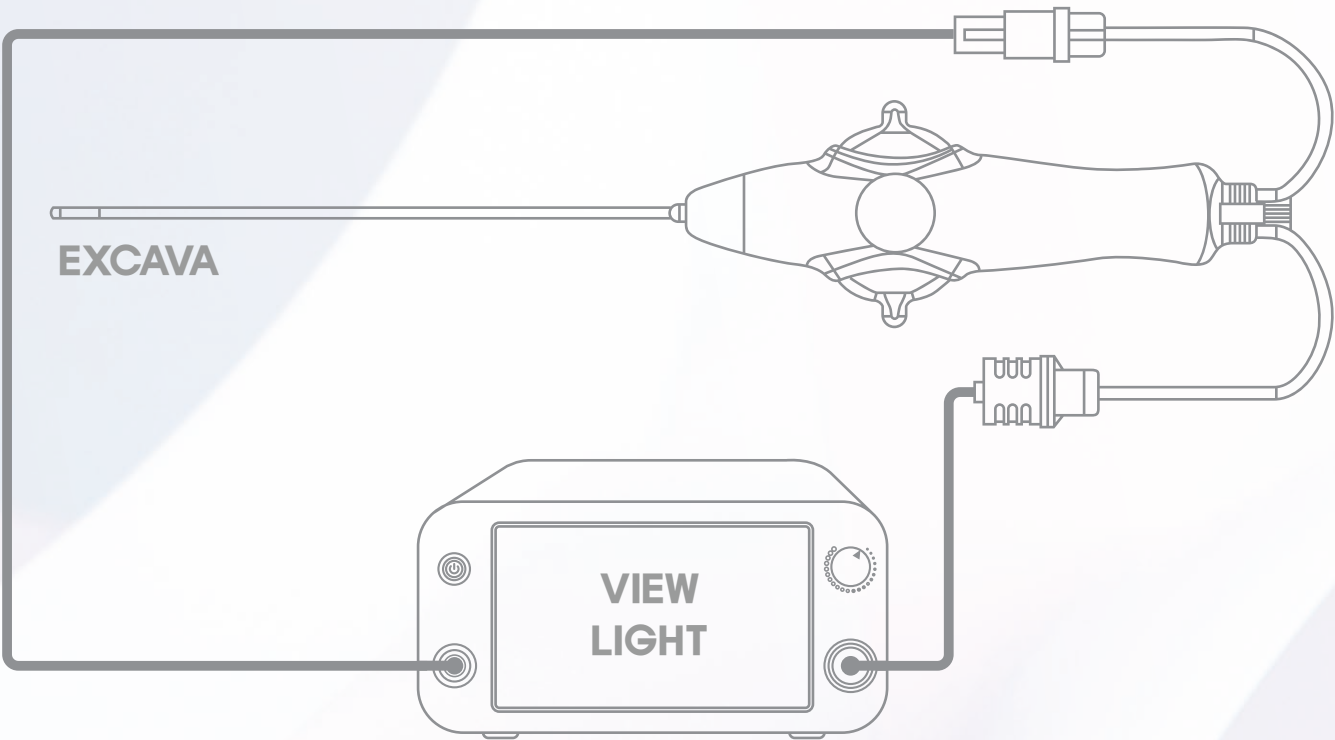


VIEW LIGHT

Specification

Type		Endoscopy Light Sources Device		LCD	Resolution	10.1inch (1200×800 pixel)
Size		330×400×170		Camera	Resolution	160k (400×400 pixel)
Power Supply	Voltage	100-240VAC		Cable	Video	2m
	Frequency	50/60Hz			Fiber Optic	2m
LED	Power	60W (15A)		Save	Power	1.5m
	CCT Range	6500k (Cold white)			USB 2.0	
	Brightness	0~100				

EXCAVA

Steerable Epidural Endoscopic Catheter

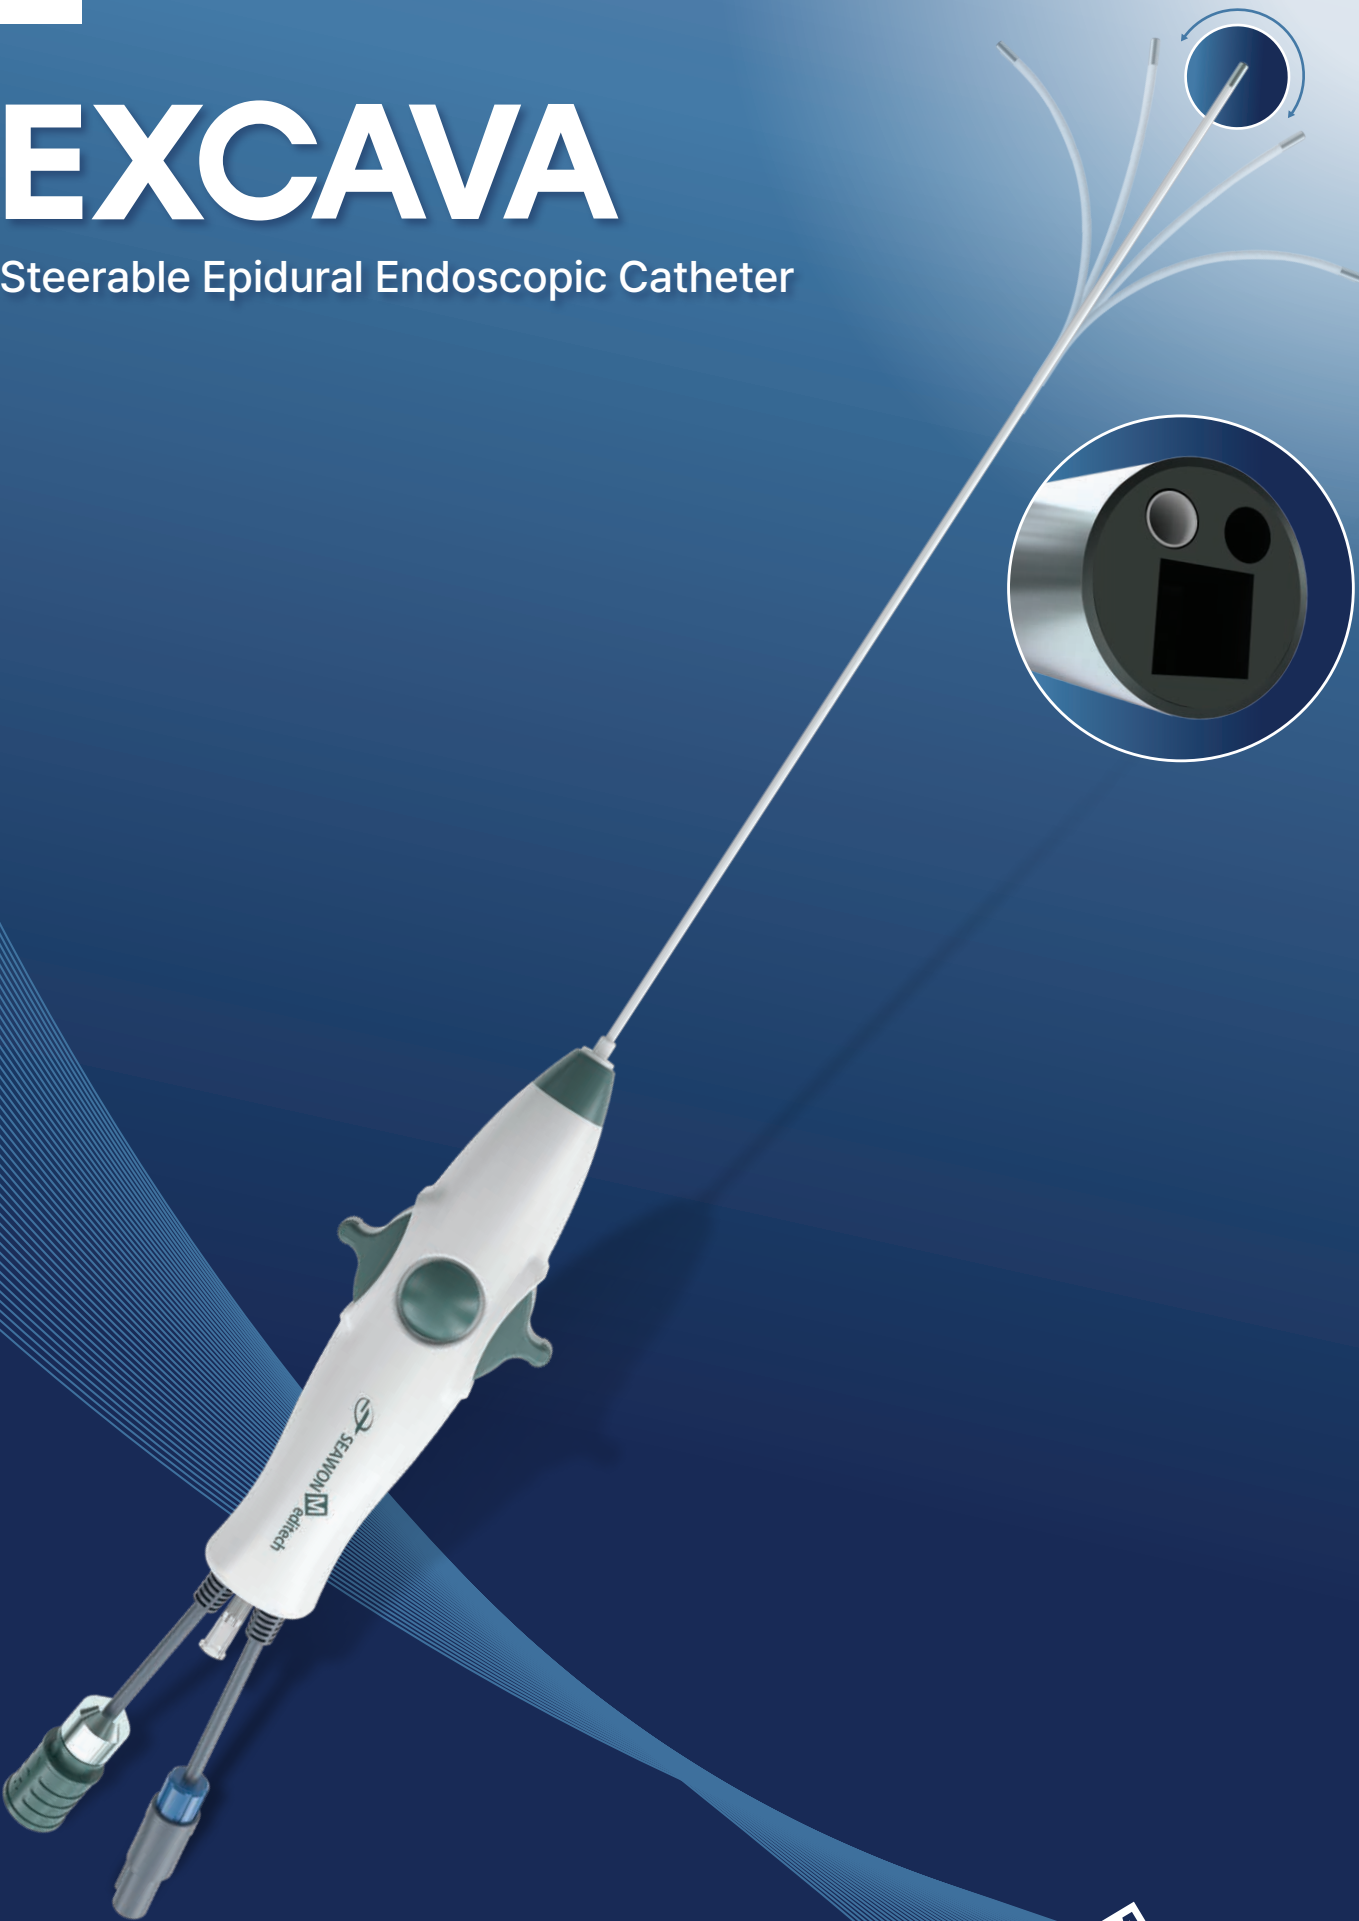

HOME PAGE

(14487) 33, Bucheon-ro 298beon-gil, Bucheon-si, Gyeonggi-do, Republic of Korea
TEL +82. 32. 684. 7072 FAX +82. 32. 684. 7075 **HOME PAGE** www.seawonmt.com
E-MAIL Domestic- jung820@seawonmt.com I Overseas -seawonmt@seawonmt.com




EXCAVA

This product is an epidural catheter generally used to inject pain relief drugs into the epidural cavity, and is a medical device combined with an in-body medical camera including a CMOS sensor.


It is a disposable medical device with an epidural needle and a pair of component medical devices used to perforate tissue before inserting the catheter insert into the body.

Power of the in-body medical camera is supplied at 3.3 Vdc from the endoscopic light source device.

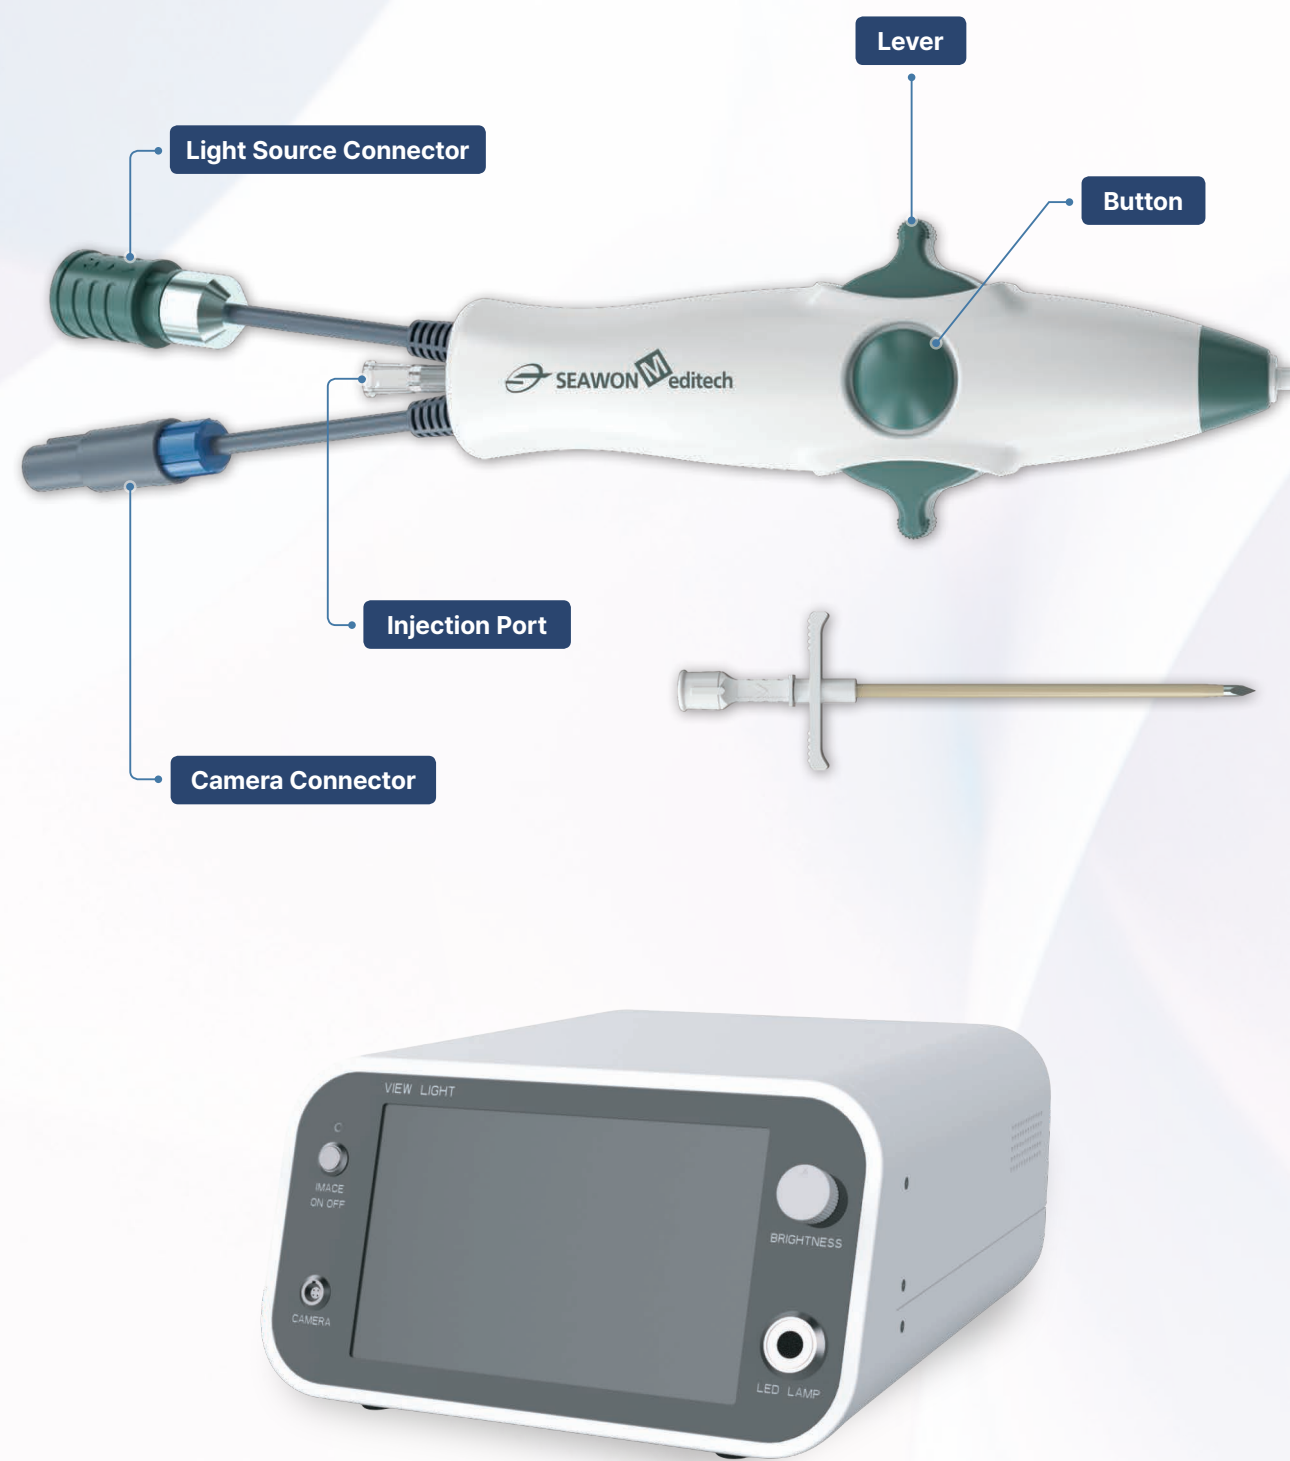

Model Spec

No	Model Name	Catheter	Needle
1	SWSD-EP-02	SWSD-EC-02	SWSD-ND-01

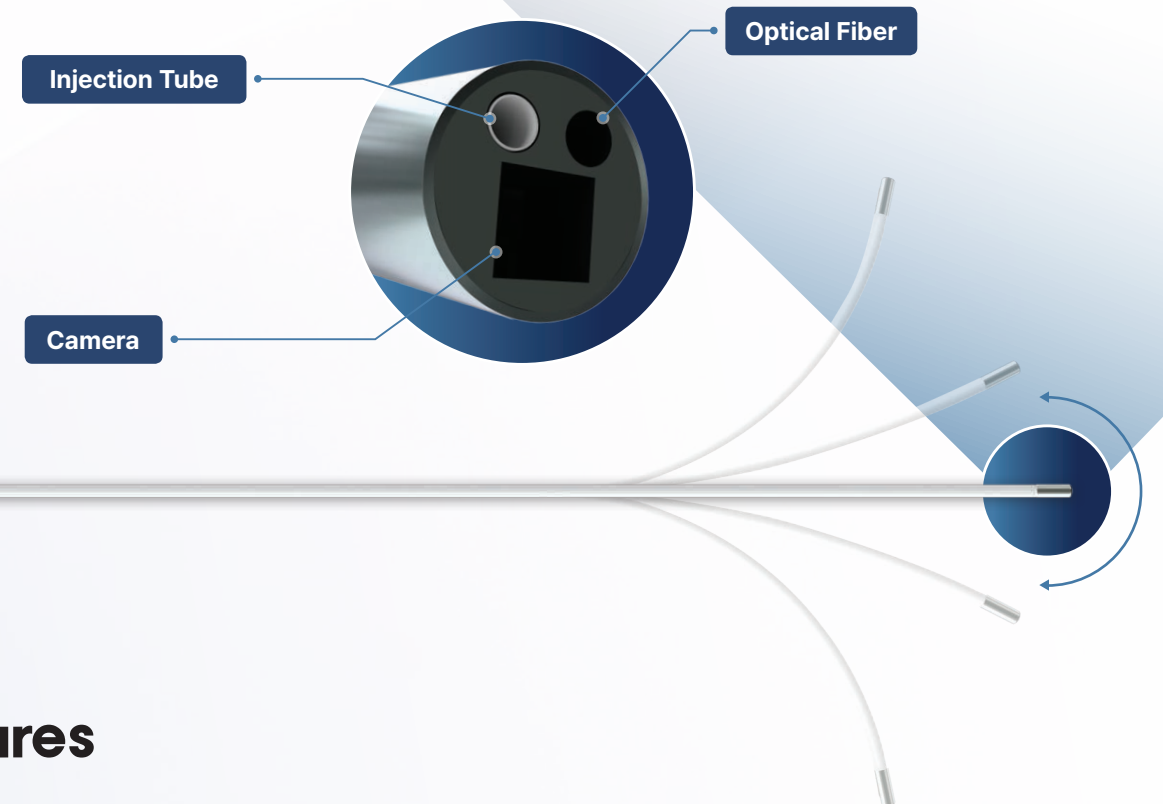

Features

01 High-Resolution



High Resolution Camera

The high-resolution enables precise diagnosis and surgical operation, with more rapid access to lesions and reducing surgery time

02 Safe



Minimally invasive

Minimum incision to reduce pain and recovery time.

Accurate treatment with visualization and illumination

Provides superior images enabling more safe operation.

03 Easy



Easy-to-use program

It uses a dedicated program

Easy-to-use ergonomic design

Ergonomic handle design easy to use

View device for illumination intensity control

Convenient for users to directly adjust illumination intensity on the view.